

## ADP1440-C06 and ADP1440-D for AXP1440

Application Note

P/N: 6806800U49C

June 2018

# Copyright

© Copyright 2018 Artesyn Embedded Technologies, Inc.

All rights reserved.

## Trademarks

Artesyn Embedded Technologies, Artesyn and the Artesyn Embedded Technologies logo are trademarks and service marks of Artesyn Embedded Technologies, Inc. All other names and logos referred to are trade names, trademarks, or registered trademarks of their respective owners. © 2018 Artesyn Embedded Technologies, Inc. All rights reserved. For full legal terms and conditions, please visit [www.artesyn.com/legal](http://www.artesyn.com/legal).

## Notice

While reasonable efforts have been made to assure the accuracy of this document, Artesyn assumes no liability resulting from any omissions in this document, or from the use of the information obtained therein. Artesyn reserves the right to revise this document and to make changes from time to time in the content hereof without obligation of Artesyn to notify any person of such revision or changes.

Electronic versions of this material may be read online, downloaded for personal use, or referenced in another document as a URL to an Artesyn website. The text itself may not be published commercially in print or electronic form, edited, translated, or otherwise altered without the permission of Artesyn.

It is possible that this publication may contain reference to or information about Artesyn products (machines and programs), programming, or services that are not available in your country. Such references or information must not be construed to mean that Artesyn intends to announce such Artesyn products, programming, or services in your country.

## Limited and Restricted Rights Legend

If the documentation contained herein is supplied, directly or indirectly, to the U.S. Government, the following notice shall apply unless otherwise agreed to in writing by Artesyn.

Use, duplication, or disclosure by the Government is subject to restrictions as set forth in subparagraph (b)(3) of the Rights in Technical Data clause at DFARS 252.227-7013 (Nov. 1995) and of the Rights in Noncommercial Computer Software and Documentation clause at DFARS 252.227-7014 (Jun. 1995).

## Contact Address

Artesyn Embedded Technologies  
2900 S. Diablo Way, Suite 190  
Tempe, Arizona 85282

## 1 Introduction

This guide provides information of the replacement of the Alarm Display Panel (ADP) in the AXP1440 (Centellis 4440) chassis. The ADP is not a defined Field Replaceable Unit (FRU) and it is a repair part only.

**Note:** Only qualified repair technicians should attempt to replace the ADP.

Along with the alarms and console connectors, the ADP contains the FRU data for the chassis. Replacing it will result in the loss of data (if not previously backed up). The FRU data may be backed up on the Shelf Manager. This should be performed by a skilled operator familiar with shelf management operations.

## 2 Backup FRU Data for the AXP1440

From the console of the Shelf Manager (SAM), use the read command to read the FRU data area of the ADP and store it in a specified file. Perform the read on both shelf managers.

The syntax is `frudatar <IPMB address> <FRU device ID> < File name>`

```
# clia frudatar 20 1 /var/nvdata/CENT4440_ShelfFruBAK.bin
```

## 3 Replace the ADP


**CAUTION:** Ensure the power is off to the AXP1440 chassis before proceeding.

**CAUTION:** Follow Electrostatic Discharge (ESD) and Safety Procedures. Artesyn strongly recommends that you use an antistatic wrist strap when replacing the ADP.

Electronic components can be extremely sensitive to ESD. After removing the component from its protective wrapper or from the shelf, place the component flat on a grounded, static-free surface. Do not slide the component over any surface.


Remove the two mounting screws that hold the ADP in place. Be careful while removing the screws as they are short and not captive.

Figure 1 Mounting Screws

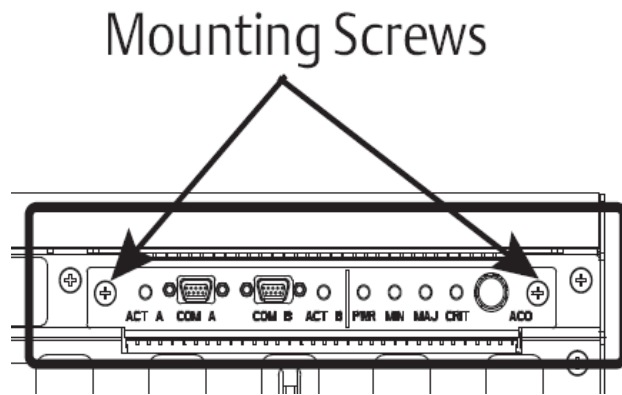

Gently pull the panel forward to expose the connector on the ribbon cable. There are levers on the sides of the connector. Push the levers to extract the ribbon cable.

Figure 2 Ribbon Cable Connector with Levers

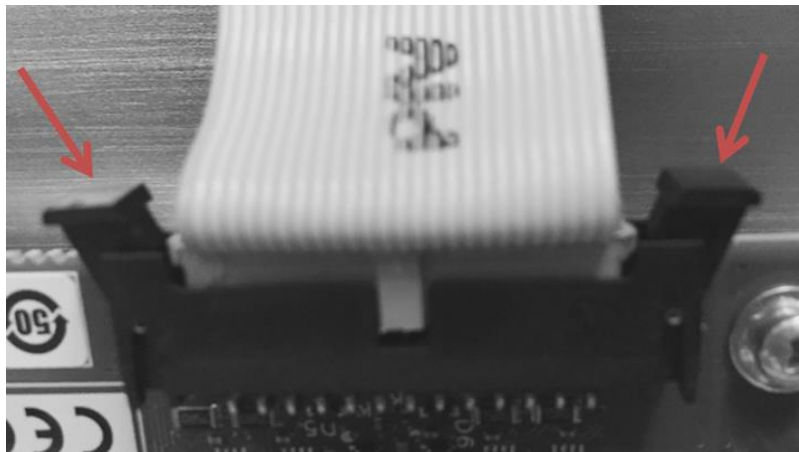

To replace the ADP, align the ribbon cable connectors and press into place. Then replace the ADP in the slot in the chassis and use the included mounting screws to fasten the ADP in place.

The chassis may now be powered up.

## 4 Restore FRU Data for the AXP1440

From each shelf manger's console, execute the following write commands to restore the FRU data from the backup.

The syntax is `clia frudataw <IPMB address> <FRU device ID> < File name>`

```
# clia frudataw 20 1 /var/nvdata/CENT4440_ShelfFruBAK.bin
```

```
# clia frudataw 20 2 /var/nvdata/CENT4440_ShelfFruBAK.bin
```



## 5 Instantiating Restored FRU Data

Power cycle the chassis or reboot both shelf managers to activate the restored FRU data. Once the system restarts, the payload boards and fan trays will transition to the active state.